

Technical Report No. 46

SACLANT ASW  
RESEARCH CENTRE

SACLANT ASW RESEARCH CENTRE  
LIBRARY COPY

A COMPACT THERMOMETER FOR THE STUDY OF MICROTHERMAL  
STRUCTURE FROM OCEANOGRAPHIC BUOYS

by

R. PESARESI and R. FRASSETTO

15 OCTOBER 1965

NATO

VIALE SAN BARTOLOMEO, 92  
LA SPEZIA, ITALY

This document is released to a NATO Government at the direction of the SACLANTCEN subject to the following conditions:

1. The recipient NATO Government agrees to use its best endeavours to ensure that the information herein disclosed, whether or not it bears a security classification, is not dealt with in any manner (a) contrary to the intent of the provisions of the Charter of the Centre, or (b) prejudicial to the rights of the owner thereof to obtain patent, copyright, or other like statutory protection therefor.

2. If the technical information was originally released to the Centre by a NATO Government subject to restrictions clearly marked on this document the recipient NATO Government agrees to use its best endeavours to abide by the terms of the restrictions so imposed by the releasing Government.

NATO UNCLASSIFIED

TECHNICAL REPORT NO. 46

SACLANT ASW RESEARCH CENTRE

Viale San Bartolomeo 92

La Spezia, Italy

A COMPACT THERMOMETER FOR THE STUDY OF MICROTHERMAL  
STRUCTURE FROM OCEANOGRAPHIC BUOYS

By

R. Pesaresi and R. Frassetto

15 October 1965

APPROVED FOR DISTRIBUTION



HENRIK NODTVEDT

Director

NATO UNCLASSIFIED





## TABLE OF CONTENTS

	<u>Page</u>
ABSTRACT	1
INTRODUCTION	2
1. ELECTRONIC CIRCUIT	4
1.1 Working Principles	4
1.2 Actual Circuit	5
2. STAGGERING	8
2.1 Principle	8
2.2 Method of combining components	9
3. CIRCUIT STABILITIES AND SENSITIVITIES	12
3.1 Long term stability	12
3.2 Short-term stability	13
3.3 Temperature sensitivity	13
3.4 Pressure sensitivity	14
3.5 Sensitivity to frequency of interrogation	15
3.6 Sensitivity to power supply voltage	15
4. PHYSICAL CONSTRUCTION	16
CONCLUSIONS AND RECOMMENDATIONS	18
FIGURES	19
TABLES	27



A COMPACT THERMOMETER FOR THE STUDY OF MICROTHERMAL  
STRUCTURE FROM OCEANOGRAPHIC BUOYS

By

R. Pesaresi and R. Frassetto

ABSTRACT

A solid-state, thermistor thermometer, of small physical size (13 cm x 14 cm), low cost (21 dollars worth of parts), and long-term stability (of the order of  $0.01^{\circ}\text{C}$  in 60 days) is described. It has been used successfully — in vertical arrays — for the study of ocean thermal microstructure in turbulent layers. Several probes can easily be plugged in on a 5 mm diam, single conductor cable that also carries the load of a special, compact oceanographic buoy. The electronic circuit is applicable to different types of sensor (i. e. current velocity, direction meters and pressure gauges).



## INTRODUCTION

A compact, oceanographic buoy system has been developed in this laboratory for the study of turbulent layer structures in transitional areas of the ocean where strong currents may be met. Sturdiness, small size, low cost and good stability were the main characteristics desired for the sensors to be suspended in vertical array from the buoy.

In this buoy system the sensors are required to make simultaneous measurements at regular intervals over long periods of time, with minimum power consumption. Among the various techniques for measuring, telemetering, and recording oceanographic variables, the most suitable seemed to be that in which a datum measurement is made proportional to a time interval between two electric pulses. This is achieved by means of a compact circuit based on an R-C timing network (the sensor providing the resistance) and a voltage sensitive switch (a unijunction transistor).

With this technique, a single conductor and sea return can be used. This permits a simple installation, in which a large number of sensors can be connected easily, both mechanically and electrically, to a single insulated wire that also forms the taut mooring cable of the buoy.

Small size was obtained by the use of miniature components and printed circuits, and by putting the circuits in epoxy resin that can be directly exposed to hydrostatic pressures. The maximum pressure reached is equivalent to a water column of 400 m. As measurements are to be made over long periods of time, stability of the circuits is an important feature, and the components have been properly selected and aged to achieve this. Among the

other characteristics that were looked for in the selection of components from manufacturers' stocks was that of minimum sensitivity to external pressure.

The buoy system is devised to permit the presentation of the pulse measurements in a sequence corresponding to the sequence of the probes on the array (first the shallowest, last the deepest). This is achieved by a staggering technique, so that each probe has its own response time, independent of the other probes. Enough pulse spacing is allowed to enable temperature-inversions at any depth to be recognised.

# 1. ELECTRONIC CIRCUIT

## 1.1 Working Principles

The working principles are illustrated in Fig. 1. Measurements are made intermittently in cycles, each of which starts when switch S connects a battery voltage E to the insulated mooring cable M and, hence, to the array of thermometers  $T_1 \dots T_n$ , (Fig. 1a). The initial surge of current induces a voltage pulse  $P_O$  in the transformer  $T_R$ , across which a magnetic tape recorder is connected. The start of the cycle is thereby recorded as a reference pulse from which all subsequent data pulses can be measured in terms of their time intervals.

The thermometer probe circuits are based on relaxation oscillators employing silicon unijunction transistors, as illustrated schematically in Fig. 1b. When the cycle starts, and battery voltage is applied to the cable, the voltage across the capacitors C1 in each thermometer circuit T start to rise. As each capacitor's voltage  $V_c$  reaches the level  $V_p$  (Fig. 1c), its associated unijunction transistor Q1 fires, C1 is discharged, and a return pulse  $P_x$  is sent back along the cable to transformer  $T_R$ , where it induces a voltage pulse that is registered on the recorder.

For any one thermometer circuit, the time interval  $t_x$  between  $P_O$  and  $P_x$  is therefore the time taken for  $V_c$  to reach the level  $V_p$ , this being dependent on the resistance  $R_T$  of the thermistor. Thus, although all the thermistor circuits start charging simultaneously, they send back independent return pulses at time intervals  $t_1, t_2 \dots t_n$  proportional to their ambient temperatures. However, as will be explained in detail later, a staggering of the time interval scale has been arranged so that there will be no confusion

when two thermometers are reading the same temperature, or when reading temperatures through an inversion.

## 1.2 Actual Circuit

The complete circuit diagram is as shown in Fig. 2, which also shows the circuits for three alternative probes: for pressure or current direction, for temperature, and for current speed. These sensor circuits can be connected, as indicated, to the input of the principal circuit shown on the left of the figure, where their variable resistance is changed into a proportional time interval between pulses. If the principal circuit was in the simple form described in Para 1.1, and illustrated in Fig. 1b, there would be nothing to prevent the capacitor C1 from starting to recharge as soon as the transistor Q1 had fired. Thus, during all the time that battery voltage was applied to the cable, there would be a continuous series of return pulses from the same circuit. The complete circuit shown in Fig. 2 is designed to prevent this, as well as to prevent each return pulse from triggering other circuits on the same cable, to stabilize and filter the incoming battery voltage, and to prevent the effects of sea water potentials and temperatures.

The diagram of the principal circuit is shown divided into two parts by broken lines. That on the right corresponds to the simple form shown in Fig. 1b, except that it is R1 that carries the discharge pulse of C1 into D1, and R2 compensates for the temperature sensitivity effects. The part on the left includes all the other additions.

During operation, the return pulse  $P_x$  — arriving through R1 — triggers the silicon controlled rectifier D1, which in turn rapidly charges the capacitor C2 through diode D3 and the external circuit.



During this process, the resistor R3 limits the current passing through D1 to a value just above its "holding current"; this in turn is kept low by the resistor R4. Thus, with D1 conducting, no further pulses from Q1 can reach the cable and be registered on the recorder.

A gate circuit, made up of diode D3 and resistor R5, prevents external pulses from other thermometers on the cable from reaching D1 and influencing its holding state. Similarly, the main thermistor circuit itself is protected from these external pulses by the filter formed by resistor R7 and capacitor C3. The thermistor circuit is also kept reasonably independent of supply voltage variations, sea water paths, sea water potentials, etc. by a voltage stabilizing circuit made up of resistors R6 and R7 and the zener diode D2.

At the end of each measurement cycle the switch S is open. In each thermometer circuit all the capacitors are discharged first through the emitter of the unijunction transistor Q1, then through the resistances  $R_T$  of the probe circuits, and hence through R1, R2 and the  $R_{bb}$  of the transistor Q1. The rectifier D1 is then closed, making the circuit ready for the next measurement cycle. The presence of the monel (used as common return) in sea water acts as a weak battery, but diode D4 prevents this charge from being received by capacitor C1.

Figure 3 shows a complete measurement cycle, both in terms of the battery voltage on the cable (upper graph) and in terms of the voltage across the recorder side of transformer TR (lower graph). The pulses  $P_1, P_2, \dots, P_n$  from n thermometer circuits are shown; the temperature recorded by each is proportional to the time interval  $(t_1, t_2, \dots, t_n)$  between its pulse and the

start pulse  $P_0$ . With the recording system at present in use it has been found that a cycle lasting 6 sec provides the required resolution for 20 probes. The cycles can be repeated at any time intervals from 20 sec to several minutes or hours, according to requirements.

## 2. STAGGERING

### 2.1 Principle

The thermistors have a negative temperature coefficient; this means that with decreasing temperature, their resistance — and the time response of the thermometers described — will increase.

Therefore, if the temperature of the sea always decreased constantly with depth (as in Fig. 4a), a group of matched thermometer circuits arranged in parallel on an array would transmit their return pulses in the order of their depth (Fig. 3). Sea temperature, however, does not continually decrease with depth — isothermal layers (Fig. 4b) and temperature inversions (Fig. 4c) are common. In isothermal water, matched thermometer circuits would send back all their return pulses at the same time; in a temperature inversion, the deeper thermometers (Y in Fig. 4c) would send back their pulses before the shallower thermometers (X in Fig. 4c), and identification would be impossible.

To avoid these difficulties a staggering method has been used, so that the thermometers transmit their return pulses at progressively delayed times according to their depth. Call  $\Delta t$  this preset interval between the return pulses of adjacent thermometers on the array when they are reading identical temperatures, and call  $S$  the sensitivity of the thermometer in  $\text{sec}/^{\circ}\text{C}$ . Then the value of  $\Delta t/S$  must be made greater than the maximum temperature inversion expected between the thermometers, if the deeper is never to send back its return pulse before the shallower. The value of  $\Delta t$  appropriate to any given temperature inversion conditions is obtained by the proper selection and combination of the thermometer circuit components.

The method of combining these different-sized components to obtain the required degree of staggering will be discussed in the next chapter. After assembly, the thermometers are calibrated and the degree of staggering verified. Figure 5 shows a sample of calibration curves and the values of  $S$  and  $\Delta t$  corresponding to one of them.

With the use of staggering it is no longer possible to use the same scale for all thermometers when interpreting the intervals between pulses as recorded temperatures. Instead, a separate scale is required for each thermometer according to its calibration curve, but this can be accomplished automatically by feeding the calibration data into the computer when the final results are being analysed.

## 2.2 Method of combining components

To obtain the required degree of staggering, slightly different values must be used for each of the principal components — the thermistor, the capacitor  $C1$ , and the unijunction transistor. There is no need to buy special components that differ by these small values, because such ranges are found within the ranges of tolerance quoted by the manufacturers of standard components. The standard components chosen were:

- |                                 |   |
|---------------------------------|---|
| for the thermistors             | - Veco 51 A 11 100 k $\Omega$<br>Tolerance of $\pm 15\%$ at 25 $^{\circ}$ C |
| for the $C1$ capacitors         | - Mylar dielectric 15 $\mu$ f, 60 v DC<br>Tolerance of $\pm 10\%$           |
| for the unijunction transistors | - 2N1671B Silicon<br>Tolerance of $\pm 20\%$                                |

In the first production, 290 capacitors, 286 thermistors and 202 unijunction transistors were bought from manufacturers' standard stocks. The frequency distribution of their deviations from quoted values was as shown in Figs. 6a, b & c respectively. If components with greater tolerance are selected, these distribution spreads can be increased and the price of components decreased.

The combination of these components to obtain the desired degree of staggering can be carried out by computer, but if a larger number of units are being assembled at once, the possibilities become too great (for 100 units there are  $10^6$  combination possibilities). In such circumstances — which would be the most usual — the quickest procedure is to combine the capacitor and unijunction transistor as described below, and then to let the computer combine these capacitor/unijunction transistor pairs with the thermistors (this reduces the possibilities handled by the computer to  $10^4$  for 100 units).

To form the capacitor/unijunction transistor pairs, the individual components are measured to within an accuracy of 1% and their values listed in increasing order. The smallest-valued capacitor is then paired with the smallest-valued transistor, and so on throughout the series. These pairs are measured in combination with a known, stable resistor. The distribution of values of the pairs is larger than the distribution of the capacitor or transistor values (theoretically it is the sum of the two distributions:  $\pm 10\%$  for the capacitors plus  $\pm 20\%$  for the unijunction transistors should give a distribution of  $\pm 30\%$  for the pairs). Figure 6d shows the result of combining the capacitors and transistors that were used for Figs. 6a and 6c respectively.

When the capacitor/transistor pairs are combined with the appropriate thermistors, a large range of values is obtained from which all the required degrees of stagger are possible.

### 3. CIRCUIT STABILITIES AND SENSITIVITIES

#### 3.1 Long term stability

Table A summarizes the differences between two calibrations made seventy days apart. The estimated instrumental error ( $\pm 5 \text{ m}^{\circ}\text{C}$ ) -- which has to be taken into account -- is due to the time measuring system (automatic time interval counter-printer) and the stability of the temperature bath (Fisher isotherm bath).

The 18 thermometer circuits in Table A were used for field measurements during twenty of the seventy days that separated the two calibrations. The remaining fifty days are to be considered as shelf time.

These records refer to the first set of thermometers, made in 1963. However, in 1964, another set was made in which the components used had not been aged. Figure 7 compares the long-term stability of these two sets. Figure 7a shows the percentage distribution of deviations recorded after 70 days with the 1963 (aged components) set; Figs. 7b & c show the percentage distributions of deviations recorded after 270 and 98 days, respectively, with the 1964 (non-aged components) set. In all three cases, the period between calibrations included a period (from 15 to 30 days) of field use.

It is seen that -- as is to be expected -- the thermometers using aged components are more stable (80% having a deviation within  $\pm 10 \text{ m}^{\circ}\text{C}$ ) than those using non-aged components. However, it is also seen that natural ageing occurs and that the stability during the second (98 day) period was proportionally greater than during the first (270 day) period. This is expressed in Fig. 7d, which compares the deviations of each individual thermometer during the two



periods. It is seen that 61% of the thermometers have a  $\Delta''/\Delta'$  relationship between 0 and +1, indicating a decreasing degree of deviation in the second period. Thus, especially if the deviations are acceptable for work during the first two years use, thermometers could more easily be made with non-aged components, as long as frequent calibrations are made during the early years.

### 3.2 Short-term stability

Short-term stability of the circuits appears to be greater than the stability of the measuring system. Table B gives the results of 20 measurements of 5 circuits, each made 5 min apart. Column (a) refers to thermometer circuits incorporating thermistors, column (b) to the same thermometer circuits where thermistors have been replaced by stable resistors.

The standard deviations  $\sigma$  and the differences  $\Delta$  between the maximum and minimum value measured are shown in each case. The differences in values of both  $\sigma$  and  $\Delta$  between columns (a) and (b) are probably due to non-homogeneities in the water of the calibration bath.

### 3.3 Temperature sensitivity

The thermometer circuits (exclusive of thermistors) are to some extent sensitive to temperature variations of the ambient. This is an effect of the individual temperature sensitivities of the three components: transistor Q1, capacitor C1, and zener diode D1 (Fig. 2).

By varying the value of resistor R2 (Fig. 2) the temperature sensitivity of the circuit can be reduced to some extent, within a given temperature range.



When a large number of components are involved, a statistical method must be used to calculate this compensation. A sample of circuits is taken and the values of  $R_2$  that minimize their temperature coefficients are measured. The average of these values is then used for the whole batch of circuits. However, before the batch of circuits is put into use, another sample is taken and tested to ensure that the chosen value of  $R_2$  has given acceptable results.

The sensitivity was found to be

$$+ \left\{ 0.48 \begin{pmatrix} +0.28 \\ -0.50 \end{pmatrix} \right\} \text{ m}^\circ\text{C}/^\circ\text{C}$$

which corresponds to

$$- \left\{ 0.24 \begin{pmatrix} +0.14 \\ -0.25 \end{pmatrix} \right\} \text{ }^\circ/\text{oo}/^\circ\text{C}$$

in the temperature range of  $13^\circ\text{C}$  to  $23^\circ\text{C}$ .

The time constant of the assembled circuits is about 3 min. Rapid ambient temperature variations can therefore introduce an error in the measurements.

### 3.4 Pressure sensitivity

The circuits are also sensitive to external pressure. The effect is felt mostly by the main capacitor; miniature air bubbles trapped between the mylar sheets decrease in volume and change its capacity.

Repeated pressure calibrations of the circuits, with a stable resistor substituted for the variable resistance of the probe, showed that the effect is different for each individual circuit but that calibration curves as a function of pressure are repeatable, within a temperature error of  $\pm 4 \text{ m}^\circ\text{C}$ .

The pressure sensitivities were measured after a short time exposure (5 min) to pressures of 10, 20, 30 and 40  $\text{kg}/\text{cm}^2$ . Beyond this latter pressure, first the transistor and then the capacitor collapsed.

Pressure sensitivities after long period of exposure exceeding two months have not yet been measured.

### 3.5 Sensitivity to frequency of interrogation

Capacitor C1 of the main circuit (Fig. 2a) takes a certain time to discharge (average 20 sec) at the end of each cycle of interrogation. The next cycle can begin only after C1 is completely discharged, if cumulative errors are to be avoided.

So far, it has not been possible to increase the interrogation rate beyond 1 cycle every 30 sec, at which rate the deviation is of the order of  $0.01^\circ\text{C}$ . Means of discharging C1 more rapidly are being investigated.

### 3.6 Sensitivity to power supply voltage

The response time sensitivity to voltage variations is within  $\pm 0.2 \text{ m}^\circ\text{C}/\text{volt}$  at the normal voltage (24v DC).

The maximum allowable deviation of  $10 \text{ m}^\circ\text{C}$  is reached below 18v DC.

#### 4. PHYSICAL CONSTRUCTION

Figure 8 shows the complete thermometer unit, as attached to the mooring cable. It is 13 cm long and 4 cm diam.; in air it weighs 120 gm and in sea water 60 gm.

The internal arrangements are shown in Fig. 9. The thermistor bid tube (1) is embedded to half its length in a capped Vinyl tube (2) filled with Araldite. The length by which it projects has been determined by tests, which show that at least 1/2 cm of the glass root below the bid must be exposed to water for effective heat dissipation. The bid is protected by a wire guard (3).

The Vinyl tube slides into a shock-absorbing rubber mounting (4) made in a conical shape so that the bid has maximum, undisturbed exposure to the current.

The thermistor is connected electrically to the rest of the circuit by flexible wires long enough to permit several renewals of this fragile unit. The rest of the circuit is potted in a PVC tube, into which the base of the rubber mount fits; to take care of the different water compressions all the intervening space is packed with Vaseline through the two buffer holes.

More than half of this tube is occupied by the main Mylar dielectric 15  $\mu$ f capacitor (C1 in the circuit diagram), held in a central position by four spacers. Below this are the remaining electronic components mounted on a circular printed circuit. The base of the tube is closed by a neoprene end-plate with a tapered wire protection. All the contents are potted in Araldite.

Electrical connections between the thermometer unit and the recorder are (1) through an electrical outlet on a single neoprene coated wire rope of high tensile strength and good flexibility and (2) by a Monel sheet riveted around the PVC tube, which acts as the conductor for sea return. The deep-sea connector for the probe passes through a tapered neoprene reinforcing sleeve.

These thermometer units have been exposed to mechanical and thermal shocks and to vibrations of up to 100 cps without any change in their original calibration curves.

Figure 8a and c show how the ground soldered contact is imbedded in the Araldite to prevent exposure to water and galvanic corrosion.

## CONCLUSIONS AND RECOMMENDATIONS

Over 100 thermometers have been made at the Centre and used for field measurements from the Centre's oceanographic buoys for periods of from 15 to 30 days at a time. They have demonstrated that, with a few improvements, the system is capable of recording temperature profiles with an accuracy of  $\pm 0.01^{\circ}\text{C}$ .

A constant error was given by pressure, but a correction appropriate to the working depth of each thermometer was applied before data processing. The maximum depth for the electronics described in this report is 400 m.

However, it has been found that with long exposure to sea pressure — after several periods of field work — the surrounding epoxy resin shows signs of fatigue, as a result of which about 30% of the thermometers used in a recent cruise (GIB V) were found to be shorted. It has therefore been decided to enclose later models in stainless steel or titanium tubes closed by PVC end-caps. This will keep the circuit at atmospheric pressure, and will also permit further reduction in the size and weight of the probes, because components can be chosen for their small size rather than for their lack of pressure-sensitivity. Because of its temperature sensitivity, the circuit will then have to be potted in a silicone compound within the metal tube. This will provide the greatest possible thermal conductivity and thereby keep the circuit at the external ambient temperature. If this is not done, there would be a risk of uncontrollable errors when there are rapid temperature variations in the water.

Although the circuit described is designed for a 30 sec minimum interrogation rate, it would require only the changing of a few critical components to make it suitable for faster rates. In such a case, of course, the recording system would have to be of a type that would permit adequate resolution.



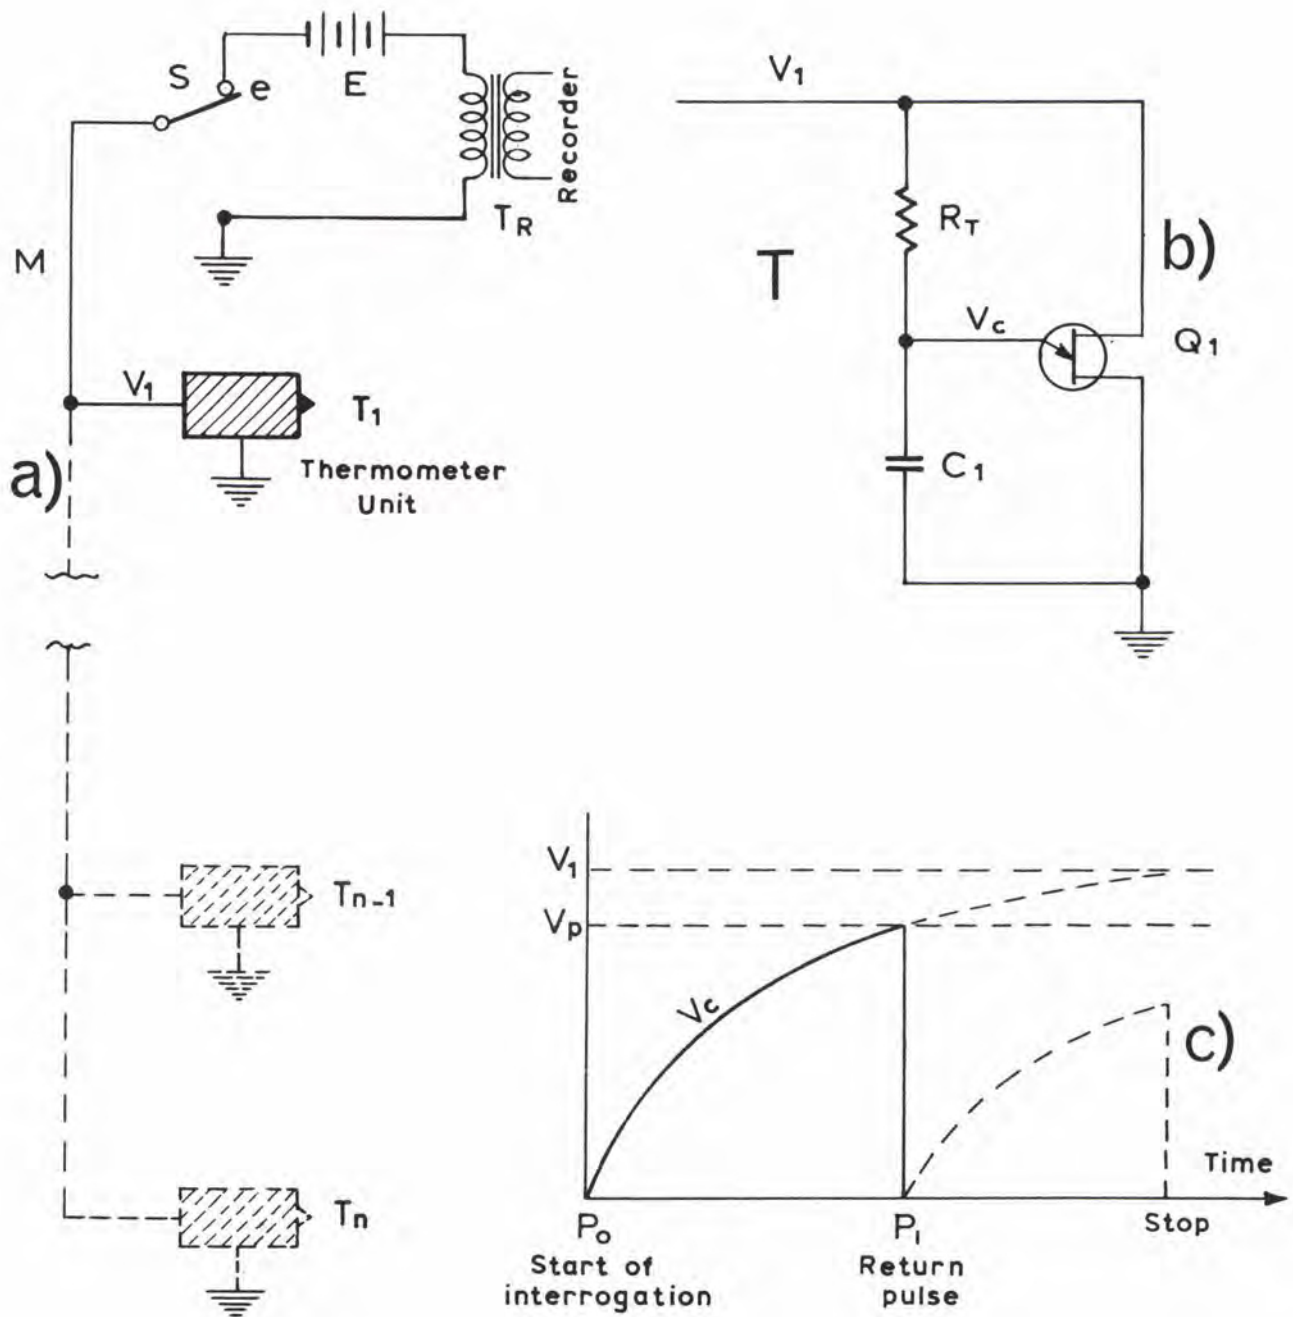


FIG. 1 WORKING PRINCIPLES OF THE ELECTRONIC CIRCUIT





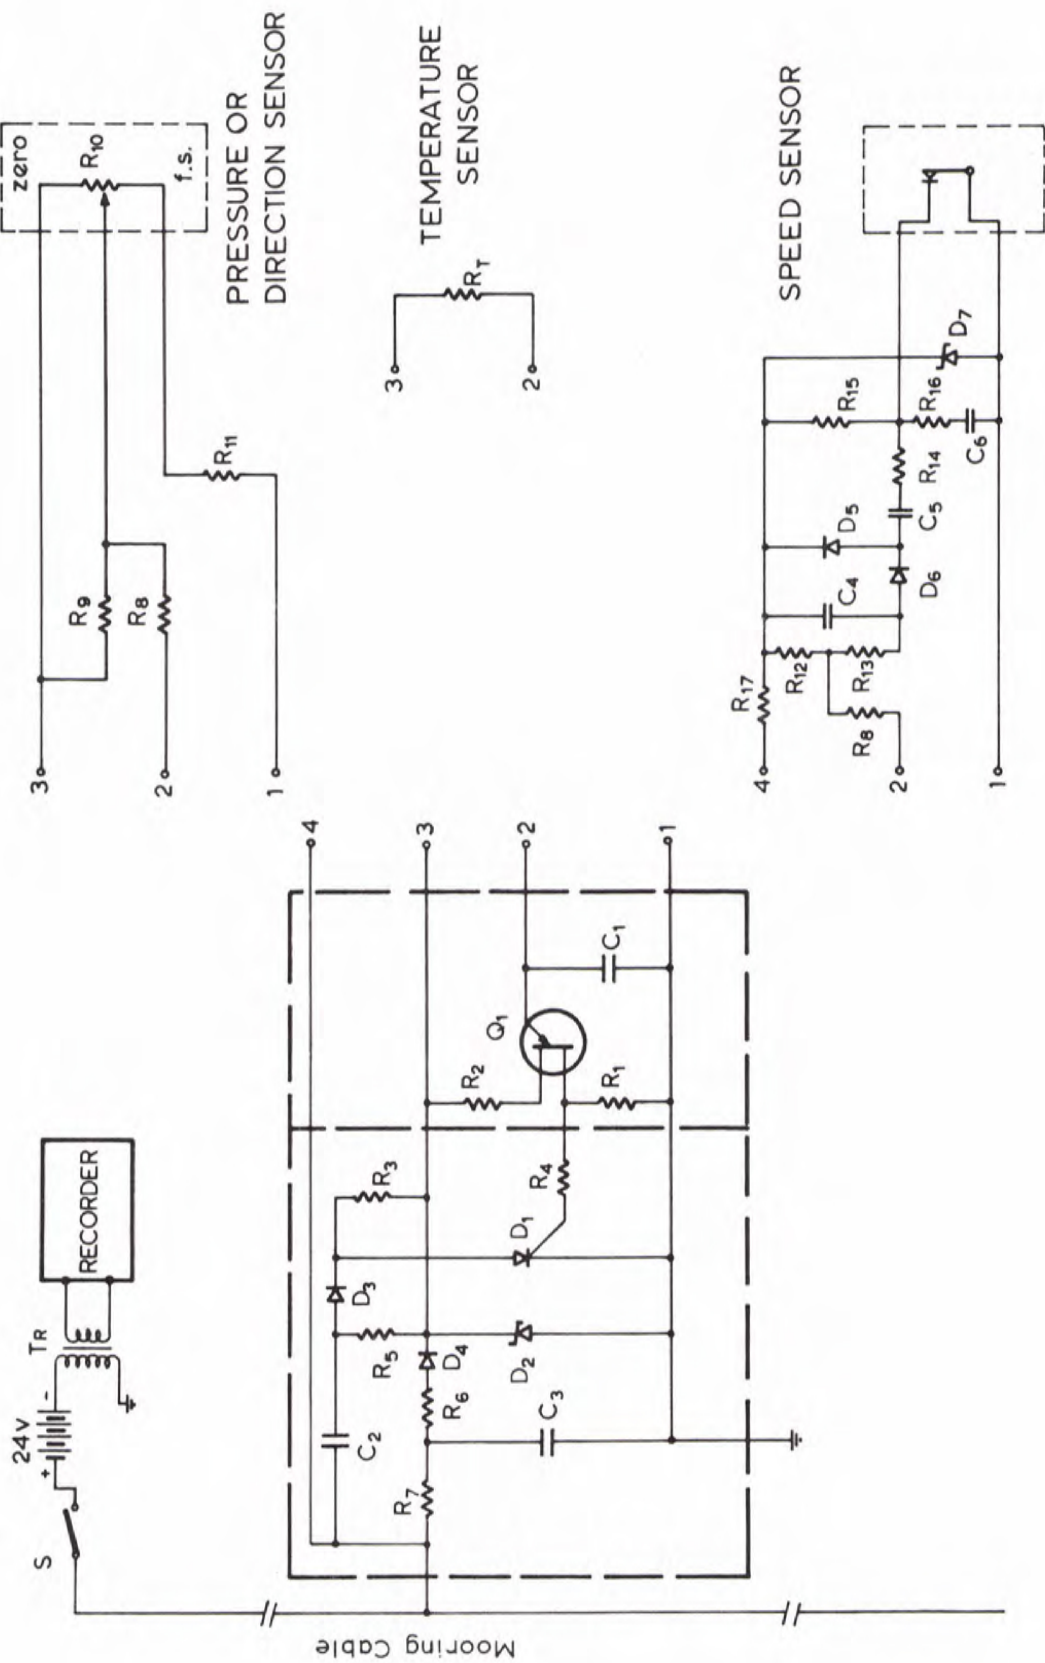


FIG. 2 CIRCUIT DIAGRAM, SHOWING THREE ALTERNATIVE SENSORS



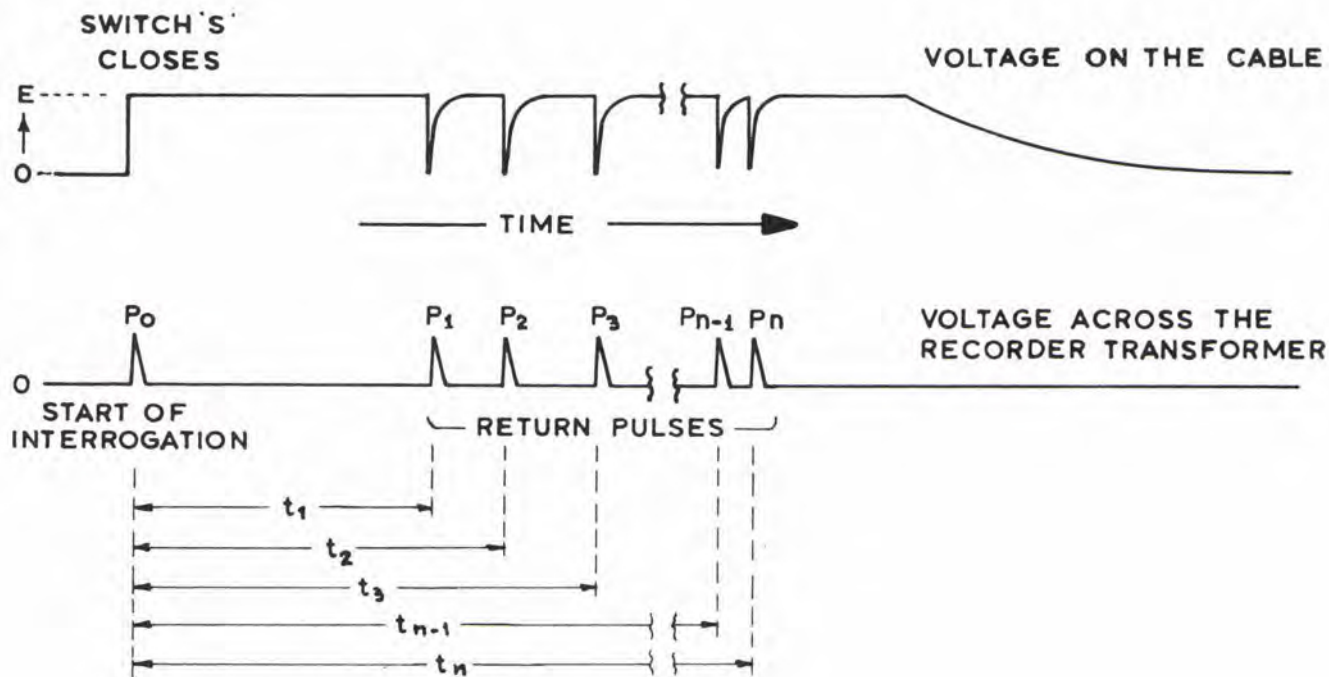


FIG. 3 COMPLETE MEASUREMENT CYCLE IN TERMS OF BOTH VOLTAGES


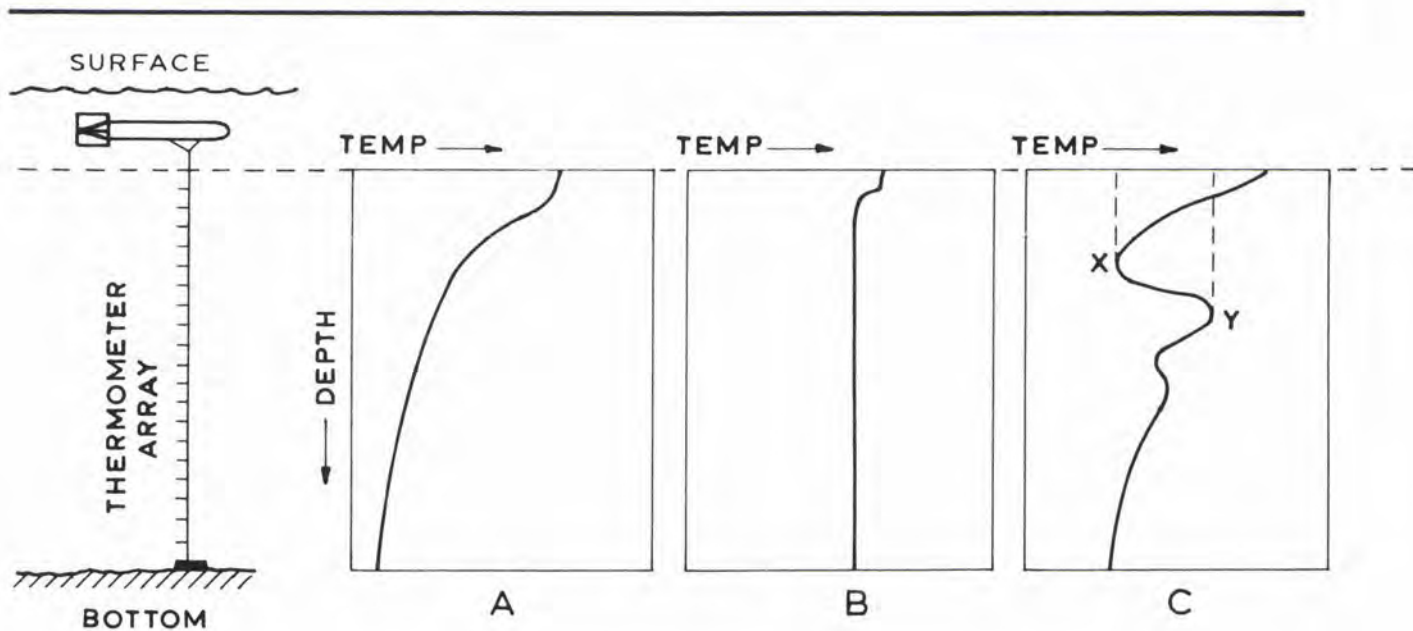


FIG. 4 MEASUREMENTS IN DIFFERENT WATER TEMPERATURE PROFILES







**FIG. 5 CALIBRATION CURVES OF THERMOMETERS**

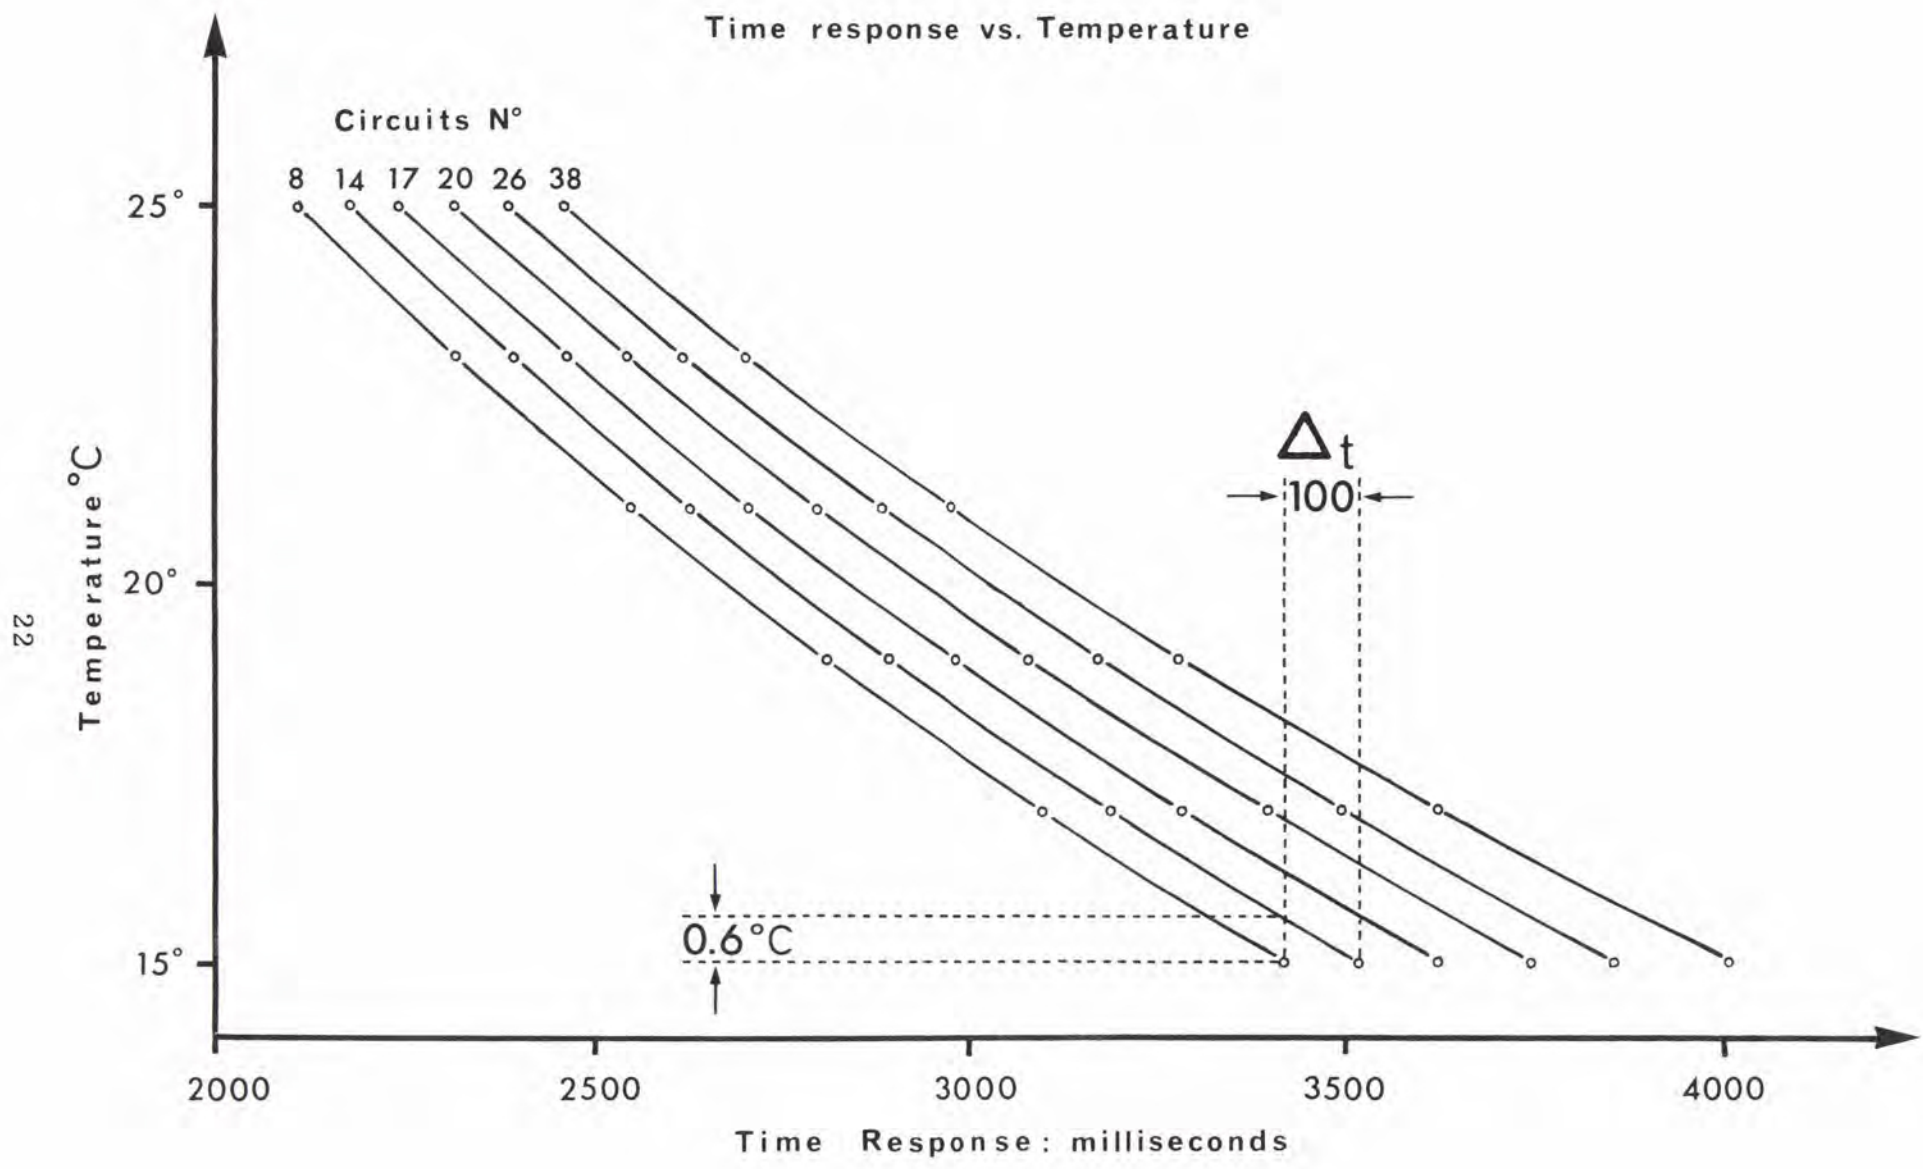


A

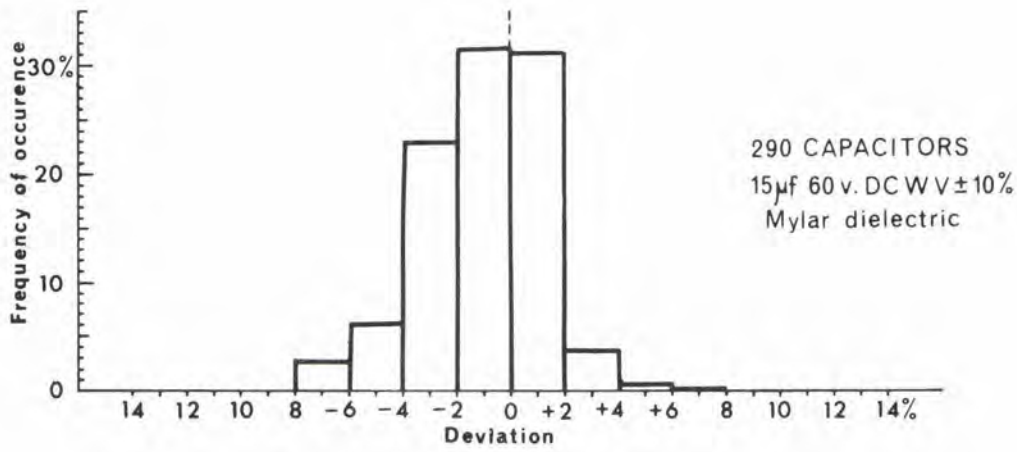

B

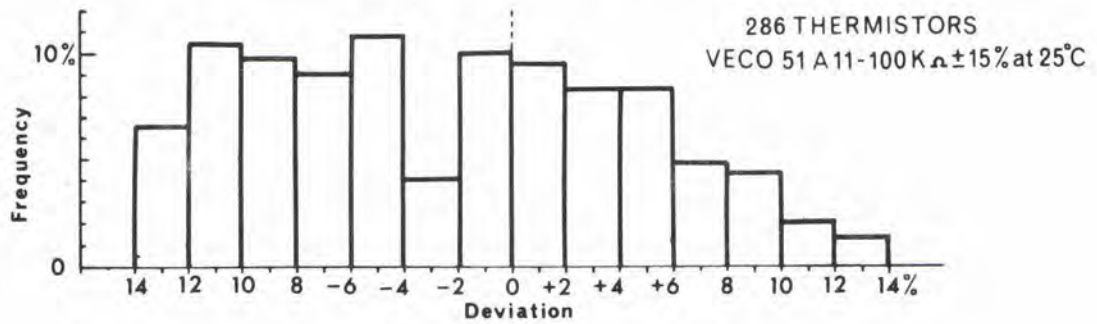

C

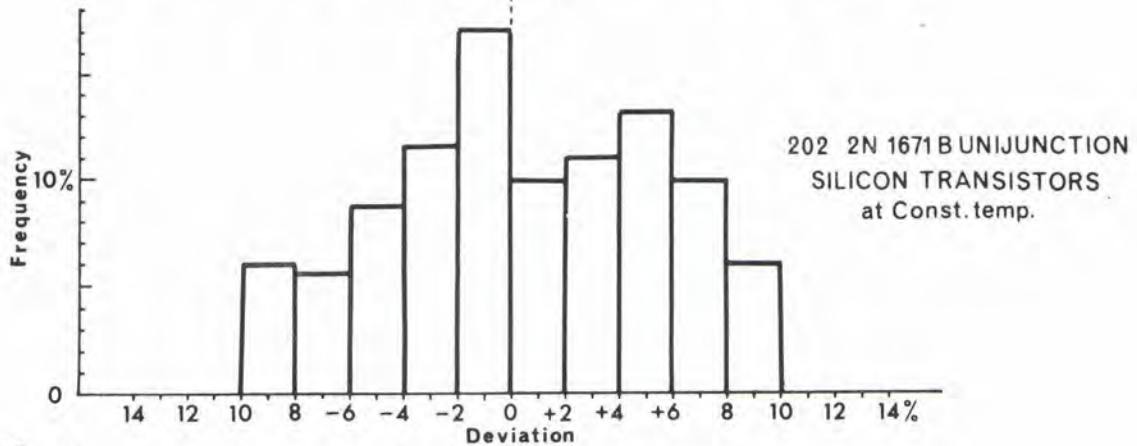

D

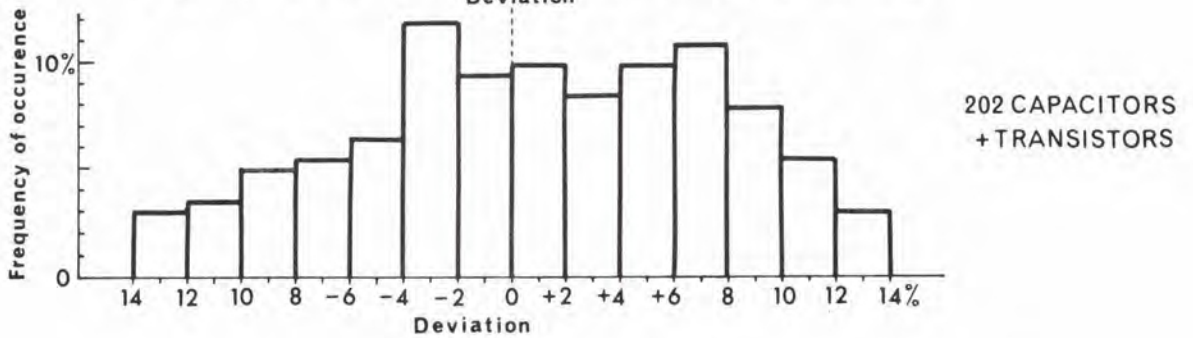


FIG. 6 FREQUENCY DISTRIBUTIONS OF DEVIATIONS FROM QUOTED VALUES





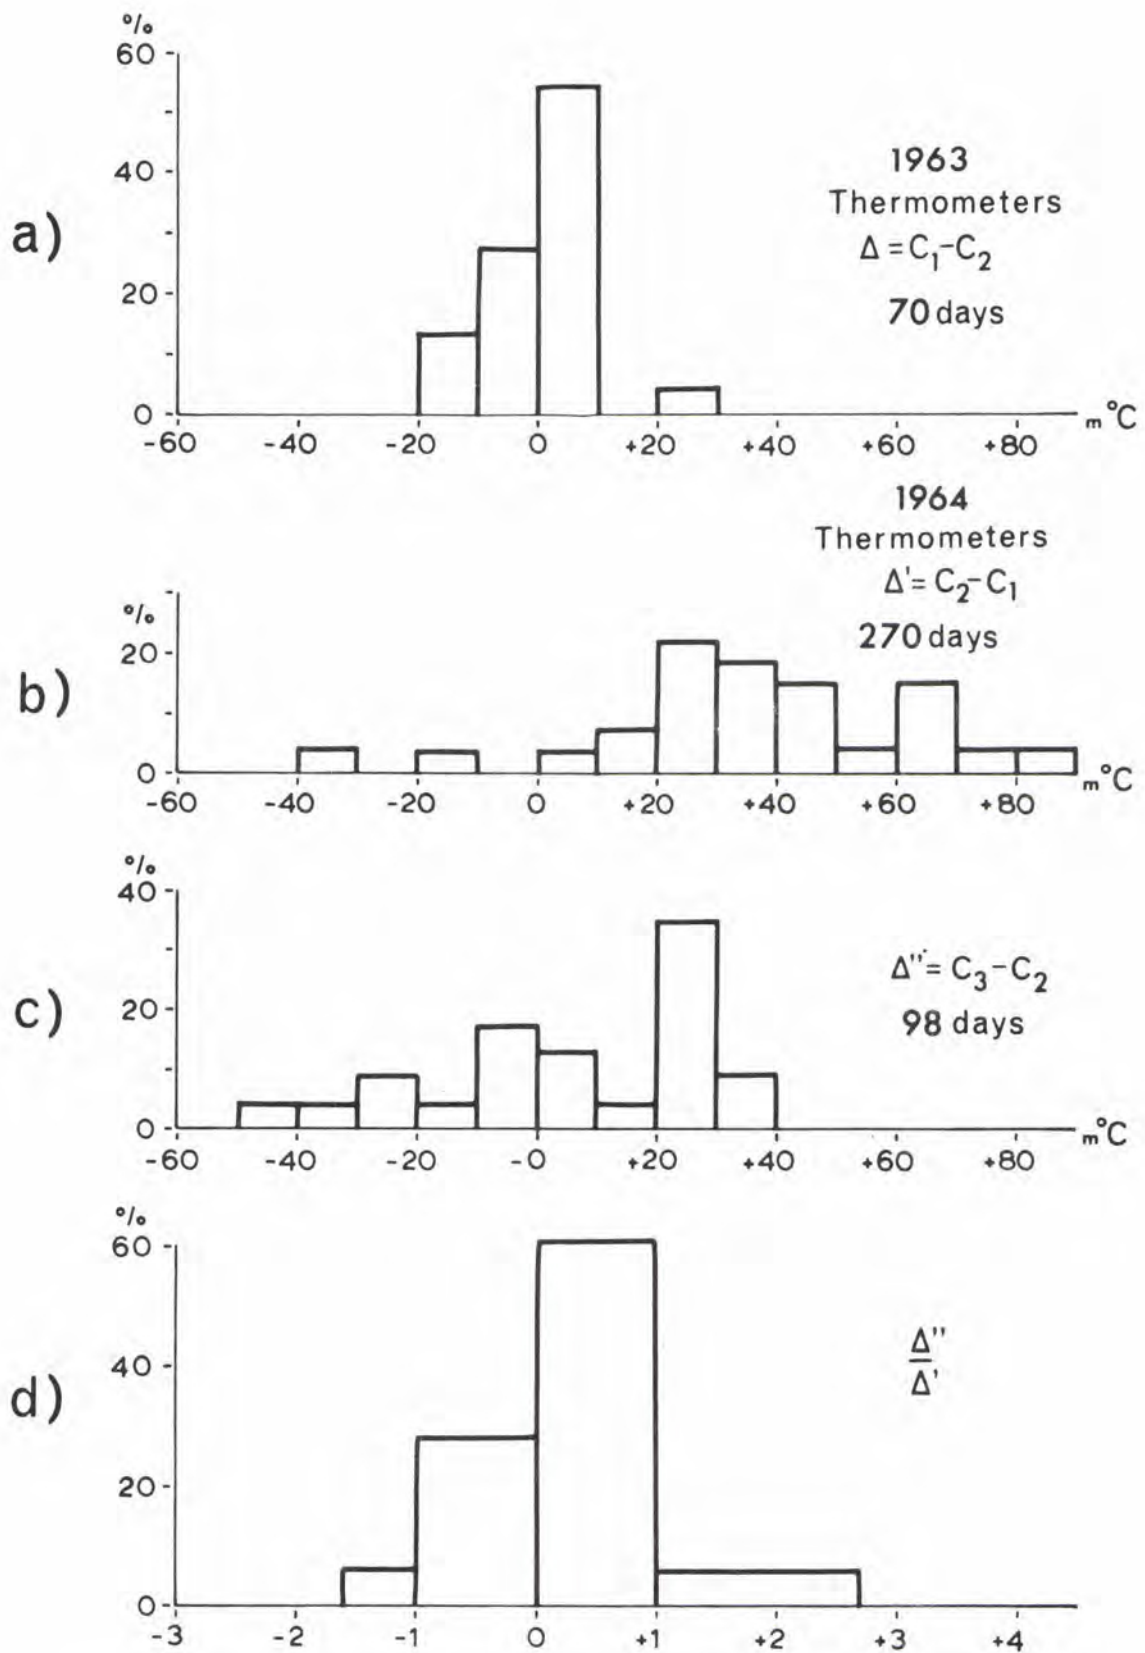



FIG. 7 COMPARISON OF LONG-TERM STABILITY BETWEEN TWO SETS OF THERMOMETERS





**FIG. 8 PHOTOGRAPH OF A COMPLETE THERMOMETER UNIT**



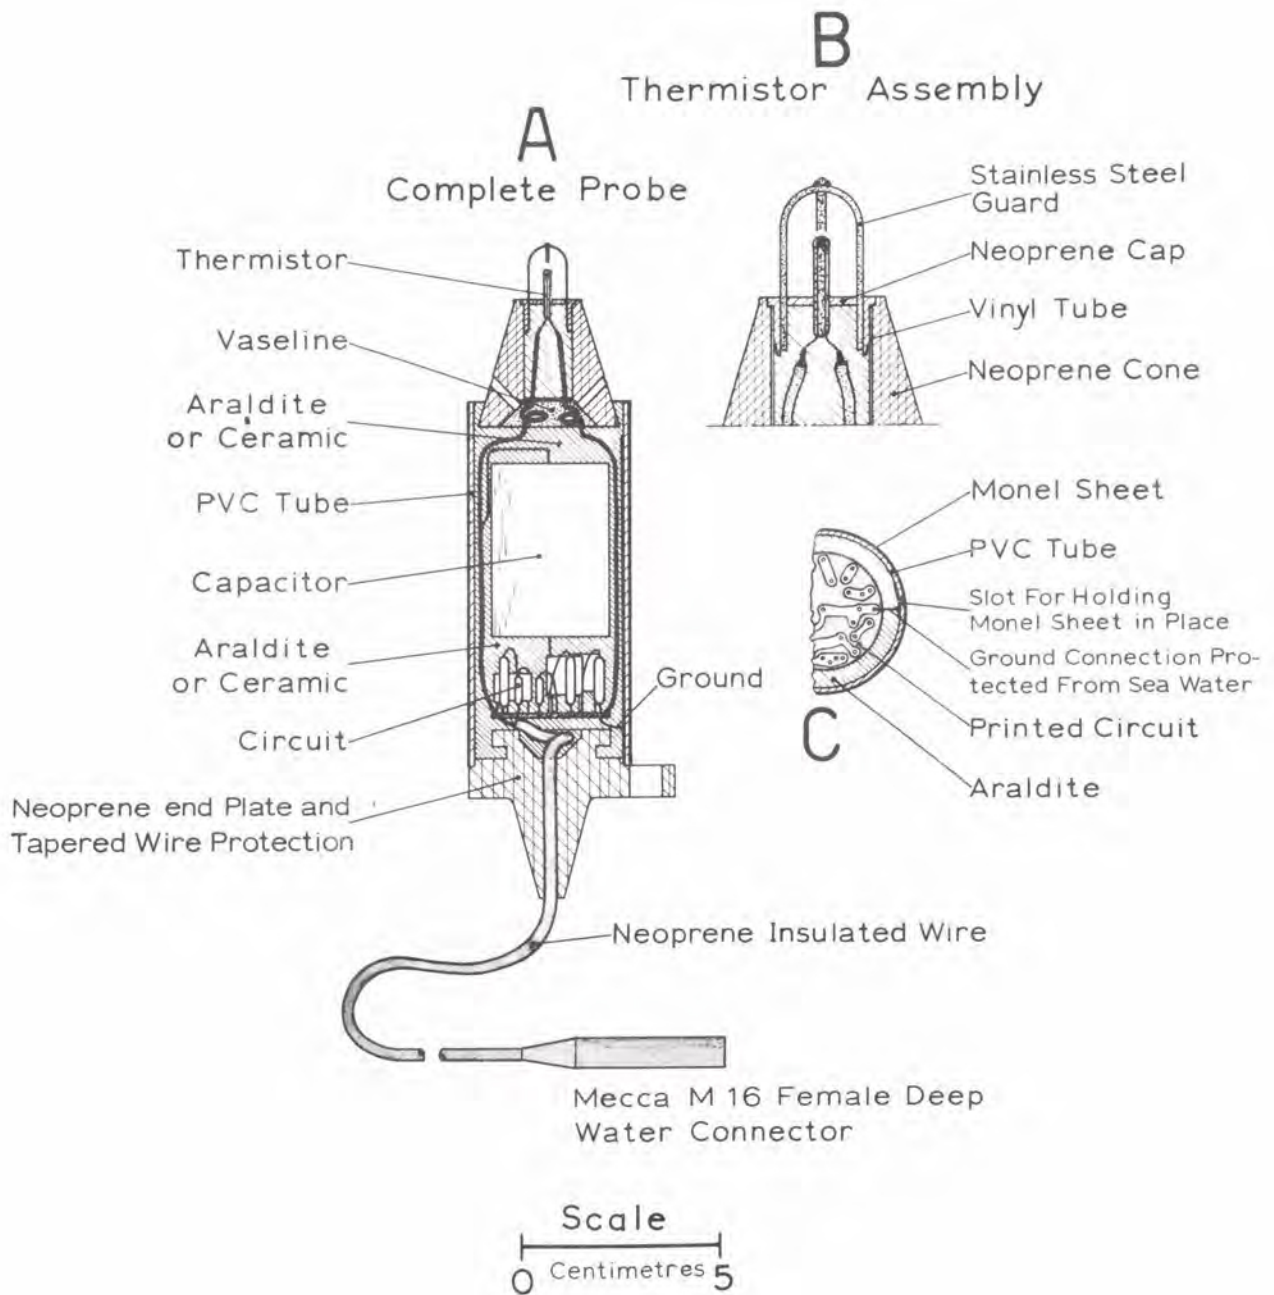

**FIG. 9 THERMOMETER – CROSS SECTION VIEW**



TABLE A  
Long - term stability

CIRCUITS	TEMPERATURE °C					
	15°	17°	19°	21°	23°	25°
<b>1</b>	1.4	4.8	0	2.6	5.0	3.2
<b>2</b>	6.4	2.8	4.6	2.6	0	-7.2
<b>3</b>	-10.0	-7.4	-6.8	0.8	-0.8	0
<b>4</b>	-16.2	-14.6	-16.0	-14.8	-16.8	-12.4
<b>5</b>	4.8	12.6	8.6	7.6	9.8	12.2
<b>6</b>	1.8	6.0	5.8	4.0	5.4	6.8
<b>7</b>	21.4	26.6	26.8	28.4	29.4	34.4
<b>8</b>	-5.2	-2.8	-1.8	-0.6	-2.2	-3.4
<b>9</b>	20.4	14.4	13.4	12.8	9.6	9.0
<b>10</b>	-1.6	-0.4	-1.4	1.0	0	4.4
<b>11</b>	-8.6	-12.0	-13.4	-11.0	-10.2	-9.8
<b>12</b>	-0.6	0	1.2	5.8	2.8	5.2
<b>13</b>	-9.0	-8.2	-9.4	-9.8	-10.0	-9.2
<b>14</b>	1.2	2.4	2.6	2.8	8.2	9.2
<b>15</b>	-4.8	-8.2	-5.8	-8.4	-9.8	-3.8
<b>16</b>	6.4	6.6	9.6	6.8	3.4	9.0
<b>17</b>	0.4	3.6	2.8	4.2	5.2	6.6
<b>18</b>	-11.6	-9.6	-12.0	-8.2	-5.2	-6.6

Deviations in temperature readings after 70 days exhibited by a typical batch of thermometers (expressed in  $m^{\circ}C \pm 5m^{\circ}C$ )






TABLE B  
Short-term stability

Circuits N°	a) with thermistor		b) with resistor	
	$\sigma$	$\Delta$	$\sigma$	$\Delta$
<b>1</b>	3.4	7.0	2.2	4.6
<b>2</b>	1.4	5.0	0.8	2.6
<b>3</b>	0.8	2.4	0.4	1.4
<b>4</b>	0.8	3.0	0.4	1.8
<b>5</b>	1.4	5.4	1.0	3.6

Deviations expressed in  $m^{\circ}C \pm 5m^{\circ}C$



# DISTRIBUTION LIST

Minister of Defense Brussels, Belgium	10 copies	Commander in Chief Western Atlantic Area (CINCWESTLANT) Norfolk 23511, Virginia	1 copy
Minister of National Defense Department of National Defense Ottawa, Canada	10 copies	Commander in Chief Eastern Atlantic Area (CINCEASTLANT) Eastbury Park, Northwood Middlesex, England	1 copy
Chief of Defense, Denmark Kastellet Copenhagen Ø, Denmark	10 copies	Maritime Air Commander Eastern Atlantic Area (COMAIREASTLANT) R. A. F. Northwood Middlesex, England	1 copy
Minister of National Defense Division Transmissions-Ecoute-Radar 51 Latour Maubourg Paris 7 <sup>e</sup> , France	10 copies	Commander Submarine Force Eastern Atlantic (COMSUBEASTLANT) Fort Blockhouse Gosport, Hants, England	1 copy
Minister of Defense Federal Republic of Germany Bonn, Germany	10 copies	Commander, Canadian Atlantic (COMCANLANT) H. M. C. Dockyard Halifax, Nova Scotia	1 copy
Minister of Defense Athens, Greece	10 copies	Commander Ocean Sub-Area (COMOCEANLANT) Norfolk 23511, Virginia	1 copy
Ministero della Difesa Stato Maggiore Marina Roma, Italy	10 copies	Supreme Allied Commander Europe (SACEUR) Paris, France	7 copies
Minister of National Defense Plein 4, The Hague, Netherlands	10 copies	SHAPE Technical Center P. O. Box 174 Stadhouders Plantsoen 15 The Hague, Netherlands	1 copy
Minister of National Defense Storgaten 33, Oslo, Norway	10 copies	Allied Commander in Chief Channel (CINCCHAN) Fort Southwick, Fareham Hampshire, England	1 copy
Minister of National Defense Lisboa, Portugal	10 copies	Commander Allied Maritime Air Force Channel (COMAIRCHAN) Northwood, England	1 copy
Minister of National Defense Ankara, Turkey	10 copies	Commander in Chief Allied Forces Mediterranean (CINCAFMED) Malta, G. C.	1 copy
Minister of Defense London, England	20 copies	Commander South East Mediterranean (COMEDSOUEAST) Malta, G. C.	1 copy
Supreme Allied Commander Atlantic (SACLANT) Norfolk 23511, Virginia	3 copies		
SACLANT Representative in Europe (SACLANTREPEUR) Place du Marechal de Lattre de Tassigny Paris 16 <sup>e</sup> , France	1 copy		

Commander Central Mediterranean (COMEDCENT) Naples, Italy	1 copy	NLR Netherlands Netherlands Joint Staff Mission 4200 Linneau Avenue Washington, D. C. 20008	1 copy
Commander Submarine Allied Command Atlantic (COMSUBACLANT) Norfolk 23511, Virginia	1 copy	NLR Norway Norwegian Military Mission 2720 34th Street, N. W. Washington, D. C.	1 copy
Commander Submarine Mediterranean (COMSUBMED) Malta, G. C.	1 copy	NLR Portugal Portuguese Military Mission 2310 Tracy Place, N. W. Washington, D. C.	1 copy
Standing Group, NATO (SGN) Room 2C256, The Pentagon Washington 25, D. C.	3 copies	NLR Turkey Turkish Joint Staff Mission 2125 LeRoy Place, N. W. Washington, D. C.	1 copy
Standing Group Representative (SGREP) Place du Marechal de Lattre de Tassigny Paris 15 <sup>e</sup> , France	5 copies	NLR United Kingdom British Defence Staffs, Washington 3100 Massachusetts Avenue, N. W. Washington, D. C.	1 copy
ASG for Scientific Affairs NATO Porte Dauphine Paris 16e, France	1 copy	NLR United States SACLANT Norfolk 23511, Virginia	40 copies
<u>National Liaison Representatives</u>		<u>Scientific Committee of National Representatives</u>	
NLR Belgium Belgian Military Mission 3330 Garfield Street, N. W. Washington, D. C.	1 copy	Dr. W. Petrie Defence Research Board Department of National Defence Ottawa, Canada	1 copy
NLR Canada Canadian Joint Staff 2450 Massachusetts Avenue, N. W. Washington, D. C.	1 copy	G. Meunier Ingenieur en Chef des Genie Maritime Services Technique des Constructions et Armes Navales 8 Boulevard Victor Paris 15 <sup>e</sup> , France	1 copy
NLR Denmark Danish Military Mission 3200 Massachusetts Avenue, N. W. Washington, D. C.	1 copy	Dr. E. Schulze Bundesministerium der Verteidigung ABT H ROMAN 2/3 Bonn, Germany	1 copy
NLR France French Military Mission 1759 "R" Street, N. W. Washington, D. C.	1 copy	Commander A. Pettas Ministry of National Defense Athens, Greece	1 copy
NLR Germany German Military Mission 3215 Cathedral Avenue, N. W. Washington, D. C.	1 copy	Professor Dr. M. Federici Segreteria NATO MARIPERMAN La Spezia	1 copy
NLR Greece Greek Military Mission 2228 Massachusetts Avenue, N. W. Washington, D. C.	1 copy	Dr. M. W. Van Batenburg Fysisch Laboratorium RVO-TNO Waaltdorplakte The Hague, Netherlands	1 copy
NLR Italy Italian Military Mission 3221 Garfield Street, N. W. Washington, D. C.	1 copy		

Mr. A. W. Ross  
Director of Naval Physical Research  
Ministry of Defence (Naval)  
Bank Block  
Old Admiralty Building  
Whitehall, London S. W. 1 1 copy

Dr. J. E. Henderson  
Applied Physics Laboratory  
University of Washington  
1013 Northeast 40th Street  
Seattle 5, Washington 1 copy

Capitaine de Fregate R. C. Lambert  
Etat Major Général Force Navale  
Caserne Prince Baudouin  
Place Dailly  
Bruxelles, Belgique 1 copy

CAPT H. L. Prause  
Søværnets Televaesen  
Lergravsvej 55  
Copenhagen S', Denmark 1 copy

Mr. F. Lied  
Norwegian Defense Research  
Establishment  
Kjeller, Norway 1 copy

Ing. CAPT N. Berkay  
Seyir Ve HDR D  
CUBUKLU  
Istanbul, Turkey 1 copy

National Liaison Officers


Mr. Sv. F. Larsen  
Danish Defense Research Board  
Østerbrogades Kaserne  
Copenhagen Ø Denmark 1 copy


CDR R. J. M. Sabatier  
EMM/TER  
2 Rue Royale  
Paris 8e, France 1 copy

Capitano di Fregata U. Gilli  
Stato Maggiore della Marina  
Roma, Italia 1 copy

LCDR J. W. Davis, USN  
Office of Naval Research  
Branch Office, London  
Box 39, Fleet Post Office  
New York, N. Y. 09510 1 copy

CDR Jose E. E. C. de Ataíde  
Instituto Hydrografico  
Rua Do Arsenal Porta H-1  
Lisboa 2, Portugal 1 copy



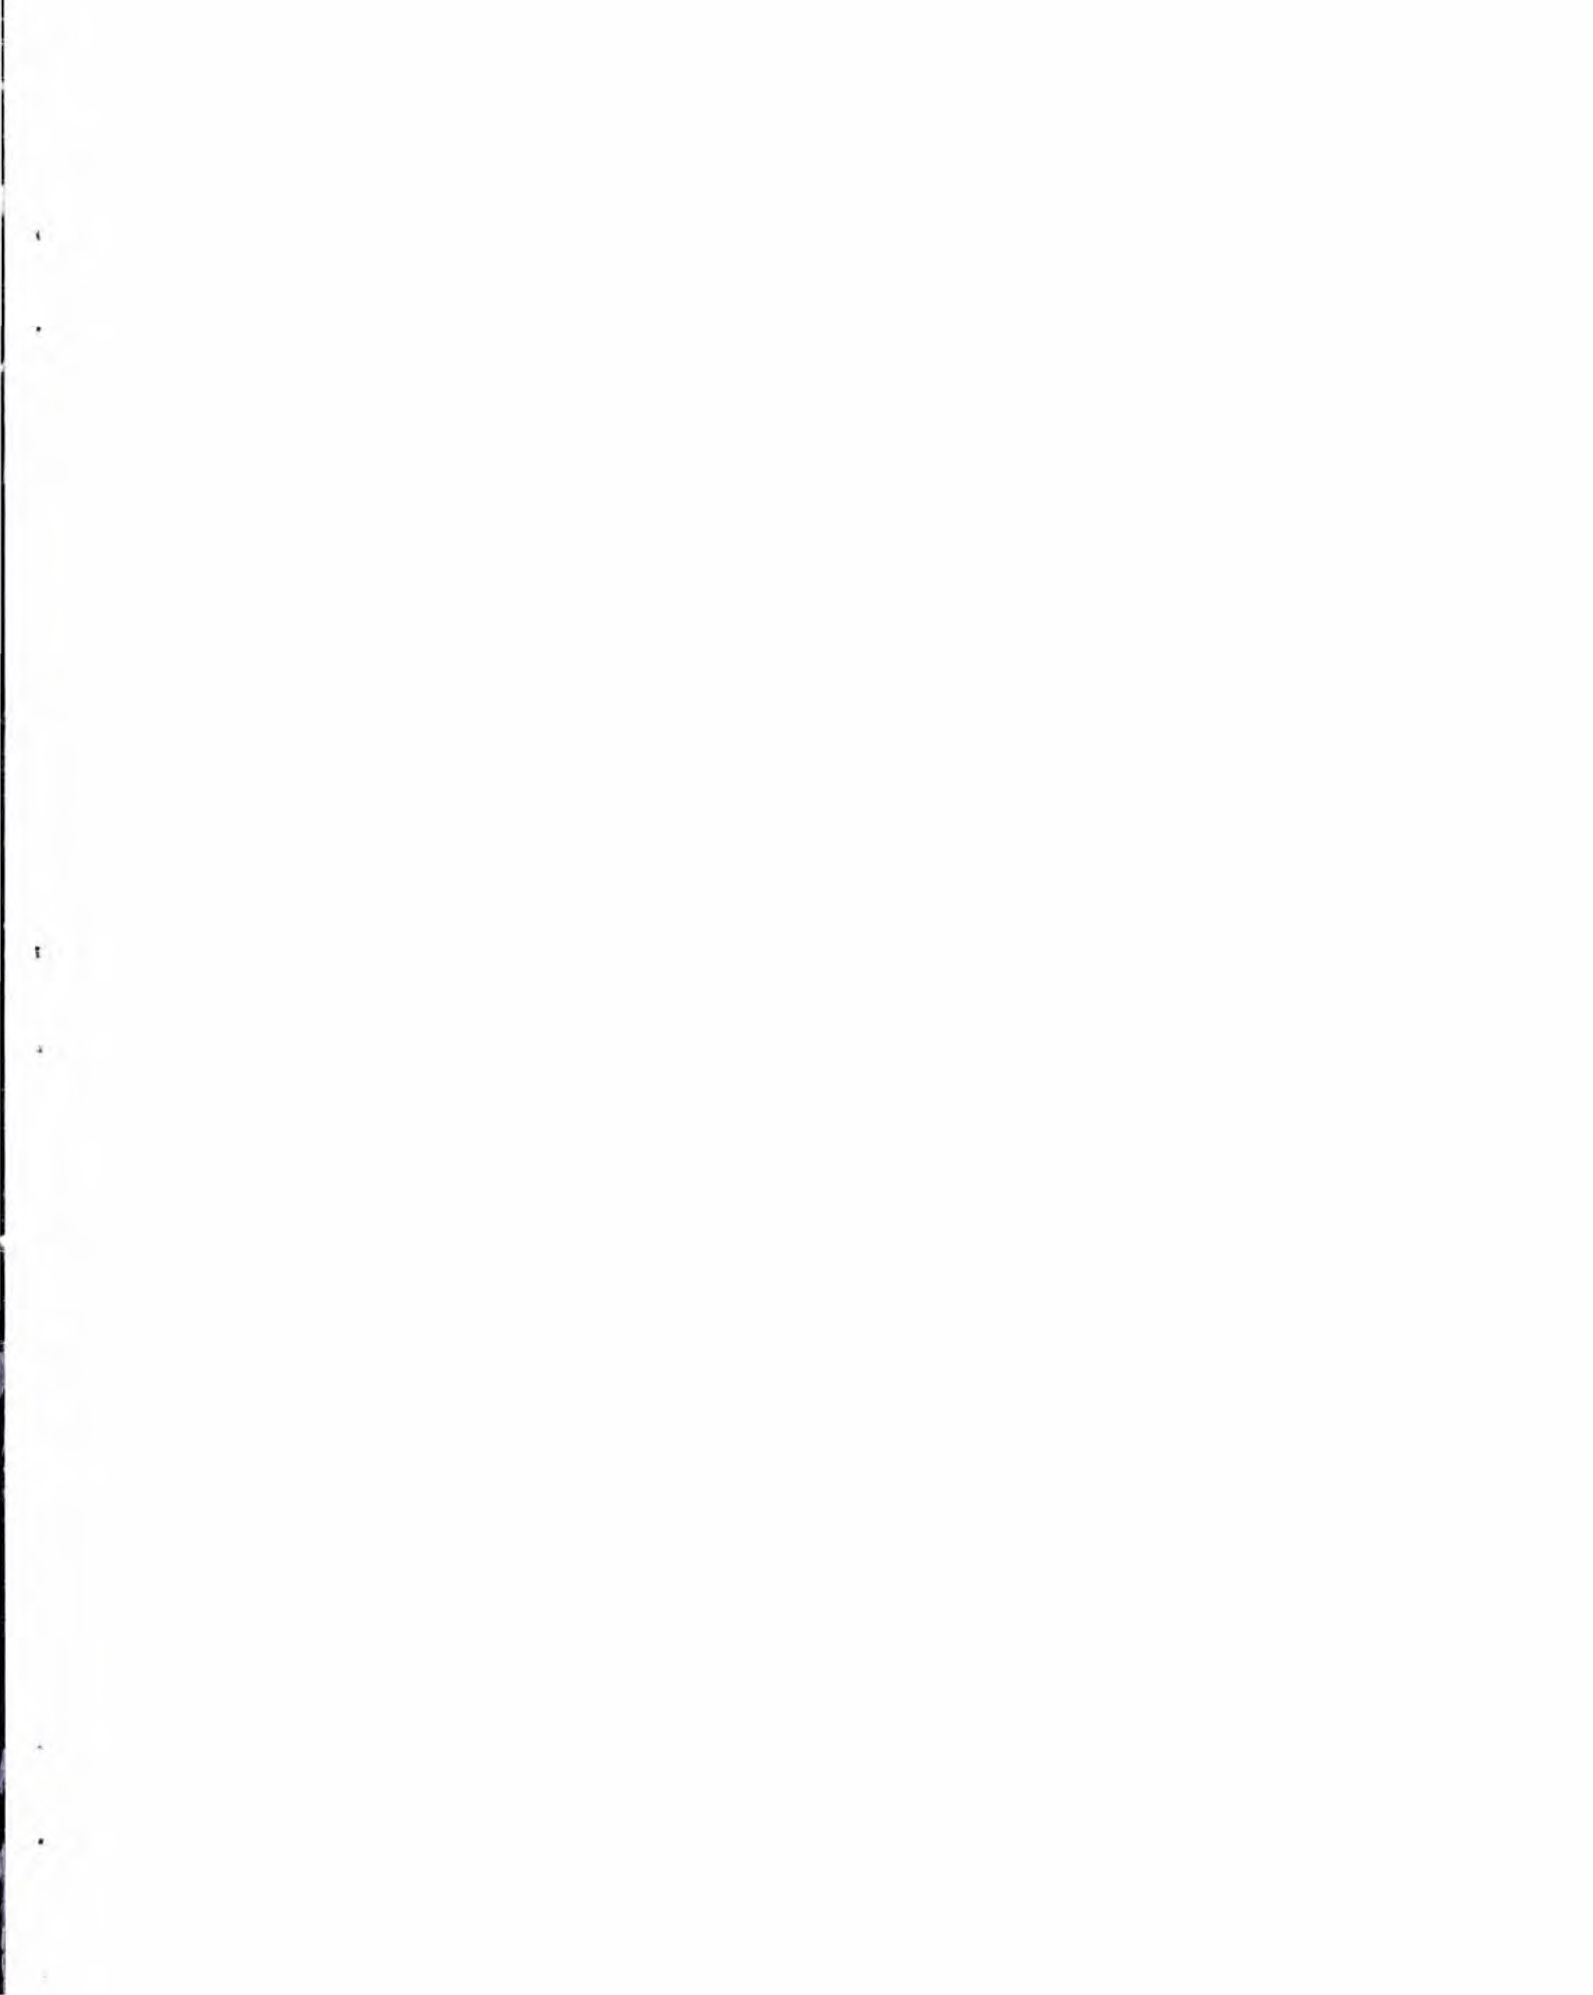

NATO UNCLASSIFIED

NATO UNCLASSIFIED